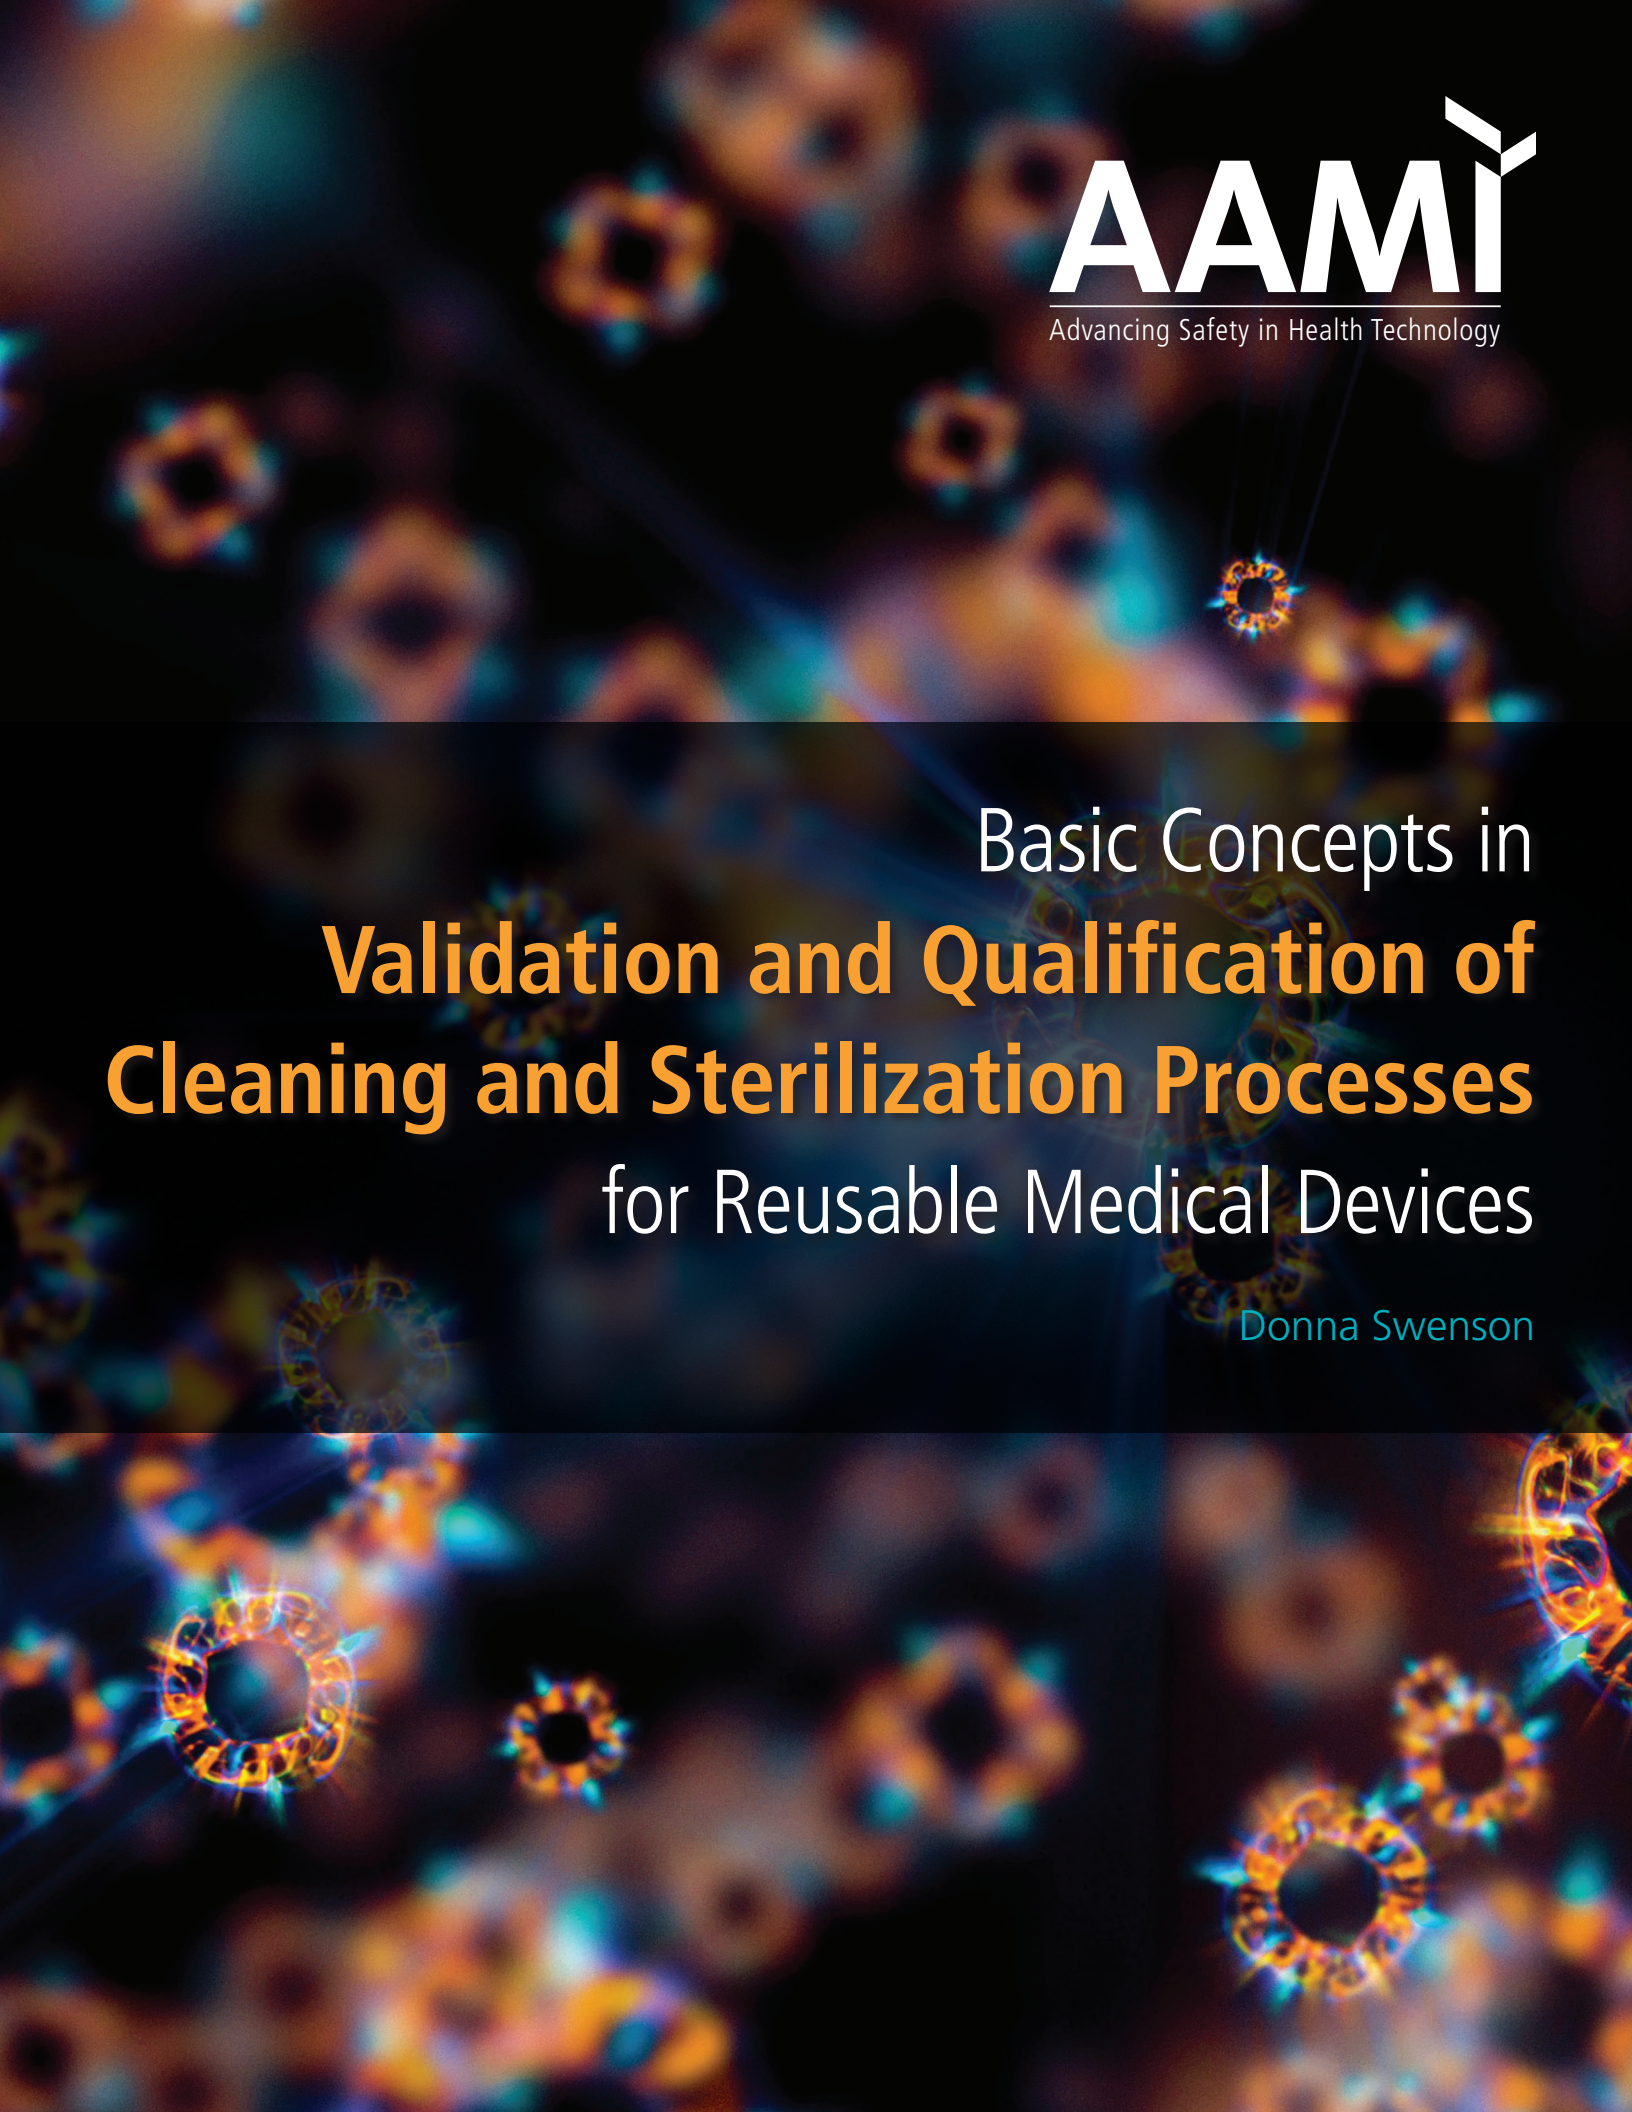

AAMI
Advancing Safety in Health Technology
Basic Concepts in
Validation and Qualification of
Cleaning and Sterilization Processes
for Reusable Medical Devices
Donna Swenson

ABOUT AAMI

The Association for the Advancement of Medical Instrumentation (AAMI), a nonprofit organization founded in 1967, is a diverse alliance of more than 9,000 members from around the world united by one critical mission—supporting the healthcare community in the development, management, and use of safe and effective medical technology. AAMI serves as a convener of diverse groups of committed professionals with one common goal—improving patient outcomes. AAMI also produces high-quality and objective information on medical technology and related processes and issues. AAMI is not an advocacy organization and prides itself on the objectivity of its work.

Published by
AAMI
901 N. Glebe Road, Suite 300
Arlington, Virginia 22203
www.aami.org

© 2021 by the Association for the Advancement of Medical Instrumentation

All Rights Reserved

Publication, reproduction, photocopying, storage, or transmission, electronically or otherwise, of all or any part of this document without the prior written permission of the Association for the Advancement of Medical Instrumentation is strictly prohibited by law. It is illegal under federal law (17 U.S.C. § 101, et seq.) to make copies of all or any part of this document (whether internally or externally) without the prior written permission of the Association for the Advancement of Medical Instrumentation. Violators risk legal action, including civil and criminal penalties, and damages of $100,000 per offense. For permission regarding the use of all or any part of this document, contact AAMI at 901 N. Glebe Road, Suite 300, Arlington, VA 22203. Phone: +1-703-525-4890; Fax: +1-703-525-1067.

Printed in the United States of America

ISBN 978-1-57020-786-0

AAMI
Advancing Safety in Health Technology

Basic Concepts in Validation and Qualification of Cleaning and Sterilization Processes for Reusable Medical Devices

Donna Swenson

Table of Contents

Page

Foreword . . . . . **vii**

Preface . . . . . **ix**

Acknowledgments . . . . . **xi**

Chapter 1. Introduction **1**

Chapter 2. Definitions and Abbreviations **3**

Chapter 3. The Science of Sterilization **9**

Introduction 9
Types of Microorganisms 9
Microbial Growth 12
Bioburden 13
Microbial Resistance 13
Microbial Lethality 13
Microbial Control 15

Chapter 4. The Quality Management System **23**

Introduction 23
General Requirements 23
Documentation Requirements 23
Management Responsibility 24
Resource Management 25
Product Realization 26
Purchasing Requirements 26
Production and Service Provisions 27
Measurement, Analysis, and Improvement 27
New Products 30
Summary 30

Page

Chapter 5. Process Validation and Verification Concepts 31
Introduction. 31
Why and When to Conduct Validation Testing 32
Validation Plans. 33
Types of Validation 36
Statistical Process Control 39
Product Design 39
Process Design 42
Installation Qualification 45
Operational Qualification 48
Performance Qualification 49
Process Control 51

Chapter 6. Cleaning Validation and Verification 53
Introduction. 53
Selection of Cleaning Method 53
Cleaning Process Validation. 56
Cleaning Process Verification 59

Chapter 7. Sterilization Validation. 69
Introduction. 69
Product Design 70
Process Design 75
Qualification Studies. 78
Installation Qualification 78
Operational Qualification 80
Performance Qualification 80
Specific Considerations for Steam Sterilization 86
Specific Considerations for Ethylene Oxide Sterilization. 95
Specific Considerations for Chemical Sterilization: Hydrogen Peroxide, Ozone, LTSF 99

Chapter 8. Product Quality Assurance Testing in Healthcare Facilities. 105
Introduction. 105
Use of Normal Production Cycles 106
Identification of Product Families and Master Products 106
Use of Chemical and Biological Indicators for Sterilization Processes 107
Placement of Master Products 108
Load Configuration 108
Drying Time and Cooling for Steam Sterilization 109
Aeration for EO Sterilization 109
Aeration for LTSF, H_2O_2, and H_2O_2/Ozone Combination Sterilization 109
Test Results for Sterilization Processes. 109
Test Results for Cleaning Processes 109
Frequency of Testing. 110

Page

Chapter 9. Human Factors Testing for Processing of Reusable Medical Devices 111
Introduction 111
Human Factors Engineering and Design Control 112
Design of Devices 112
Design Principles 113
Material Characteristics 114
Design of Processing Procedures 114
Processing Personnel 116
Design of Processing Instructions 116
Education, Training, and Competency 117
Validation 117

Bibliography 119
Cited References 119
Other Resources 121

Annexes
A Sample Protocol for Operational Qualification of a Sterilizer 125
B Sample Outline of a Cleaning Process Validation Protocol 127
C Sample Outline of a Cleaning Process Validation Report 129
D Sample Outline for a Formative Human Factors Usability Study 131

Figures
1 Microbial Lethality Measures 15
2 Example of an Audit Form 29
3 Sample Outline of a Validation Master Plan 35
4 Sample Outline of a Validation Protocol 36
5 Sample Installation Drawing Showing Minimum Service Clearance 46
6 Control Chart for Cannula Inner Diameter 52
7 Manual Cleaning 55
8 Visual Inspection of an Instrument 63
9 Visual Inspection of an Instrument with Magnification Shown on a Computer Screen . . . 63
10 Various Types of Sterilization Packaging 74
11 Sample Checklist for Installation of a Steam Sterilizer 89
12 Sample Checklist of Service and Utility Requirements for a Medium-Size Healthcare Steam Sterilizer 90
13 Diagram of Data Logger Placement for Empty-Chamber Heat Distribution Study 94
14 Sample Checklist for Installation of an EO Sterilizer 98
15 Sample Checklist for Installation of an H_2O_2 Sterilizer 101

Tables
1 Exponential Growth of Unicellular Organisms 12
2 Sterility Assurance Level/Spore Log Reduction 14
3 Additional Reprocessing Criteria and Issues 41
4 Sample Service/Utility Requirements for an Installation Qualification 47

Page

Tables (continued)

5 Laboratory Residue Detection Methods 57
6 Acceptance Criteria 58
7 In-Use Tests Available to Assess Efficacy of Cleaning of Medical Devices 60
8 In-Use Tests Available to Assess Efficacy of Wash Processes/Automated Wash Equipment Used for Medical Device Reprocessing 61
9 IES-Recommended Illuminance Levels for Work Environments 64
10 Soils Removed by Detergents of Various pH Levels 67
11 Terminal Sterilization Process Development 82
12 Considerations for Placement of BIs and CIs in Master Products 85
13 Sample Product Density Calculations 87
14 Time and Temperature Parameters for Gravity-Displacement Steam Sterilization Cycles in Healthcare Facilities 88
15 Time and Temperature Parameters for Dynamic-Air-Removal Steam Sterilization Cycles in Healthcare Facilities 88
16 Steam Quality Requirements for Sterilization 91
17 Contaminants in Condensate Measured at the Steam Inlet to the Sterilizer to Be Considered in Relationship to the Corrosion of Materials (for Clean Steam) 92
18 Contaminants in Condensate from Steam Used by the Sterilizer to Be Considered in Relation to Contamination of the Load 93
19 Operational Qualification Performance Tests 95
20 Examples of User Demographics 114
21 A Simple Task Analysis for Automated Washer Cleaning of a Needle Holder 115