INTERNATIONAL STANDARD

ISO 19614

First edition
2017-05

Traditional Chinese medicine — Pulse graph force transducer

Médecine traditionnelle chinoise — Transducteur d'intensité du pouls

Reference number
ISO 19614:2017(E)

© ISO 2017



COPYRIGHT PROTECTED DOCUMENT

© ISO 2017, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword ... **iv**

1 Scope ... **1**

2 Normative references ... **1**

3 Terms and definitions ... **1**

4 Symbols ... **8**

5 Classification ... **8**

6 Test conditions and preparation ... **8**
6.1 Test conditions ... 8
6.1.1 Environmental conditions ... 8
6.1.2 Loading condition ... 9
6.1.3 Preconditioning ... 9
6.1.4 Warm-up ... 9
6.2 Preparation ... 9

7 Requirements ... **10**
7.1 Labelling ... 10
7.1.1 Product marking ... 10
7.1.2 Technical description ... 10
7.2 Rated load (F_n) ... 10
7.3 Temperature characteristics ... 11
7.4 Geometric dimension of transducer applied plane ... 11
7.5 Input resistance (R_i) ... 11
7.6 Output resistance (R_o) ... 12
7.7 Transducer output independence ... 12
7.8 Full scale span error (*Fs*) ... 12
7.9 Terminal linearity error (*L*) ... 12
7.10 Hysteresis (*H*) ... 13
7.11 Repeatability (*R*) ... 13
7.12 Creep (*Cp*) ... 13
7.13 Offset stability (*Zs*) ... 14
7.14 Offset temperature drift (*Zt*) ... 14
7.15 Sensitivity temperature drift (*St*) ... 14
7.16 Eccentricity (*Sz*) ... 15
7.17 Overload (*Ov*) ... 16
7.18 Vibration, impact and temperature influence ... 16
7.19 Fatigue life ... 16
7.20 Biological evaluation ... 17

Annex A (informative) **Transducer examples** ... **18**

Bibliography ... **20**

© ISO 2017 – All rights reserved

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 249, *Traditional Chinese medicine*.

© ISO 2017 – All rights reserved

Traditional Chinese medicine — Pulse graph force transducer

1 Scope

This document specifies the technical requirements, classification and test method for a pulse graph force transducer, hereafter referred to as transducer.

It only applies to pulse graph acquisition over the patient's radial artery based on TCM pulse condition requirements.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 10993-1, *Biological evaluation of medical devices — Part 1: Evaluation and testing within a risk management process*

IEC 60068-2-6, *Environmental testing — Part 2-6: Test Fc: Vibration (sinusoidal)*

IEC 60068-2-14, *Environmental testing — Part 2-14: Tests — Test N: Change of temperature*

IEC 60068-2-27, *Environmental testing — Part 2-27: Tests — Test Ea and guidance: Shock*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

— ISO Online browsing platform: available at http://www.iso.org/obp

— IEC Electropedia: available at http://www.electropedia.org/

3.1
pulse graph force transducer
transducer that can detect pulsation of the radial artery and its peripheral tissues as a mechanical quantity and convert it into an electrical signal output according to a certain pattern for the purpose of TCM pulse condition acquisition

Note 1 to entry: Transducers involved in this document only refer to pressure or force transducers.

3.2
calibration
process of recording input/output data through applied standard mechanical quantities to determine the performance of transducers

Note 1 to entry: The calibration unit of transducers may be the unit of either pressure or force.

© ISO 2017 – All rights reserved

3.3
radial artery pulse graph
pulse graph
electrical signal waveform converted from peripheral vascular pulsation at the radial artery, expressed in time-amplitude coordinates, hereafter referred to as pulse graph


3.4
effective plane
plane of transducers with the sensitivity during radial artery pulsation acquisition

Note 1 to entry: See Figure 1.

3.5
auxiliary plane
plane with no sensitivity and lower than the *effective plane* (3.4) of transducers

Note 1 to entry: See Figure 1.

3.6
applied plane
contact plane of transducers with patients during pulse graph acquisition, including the *effective plane* (3.4) and *auxiliary plane* (3.5)

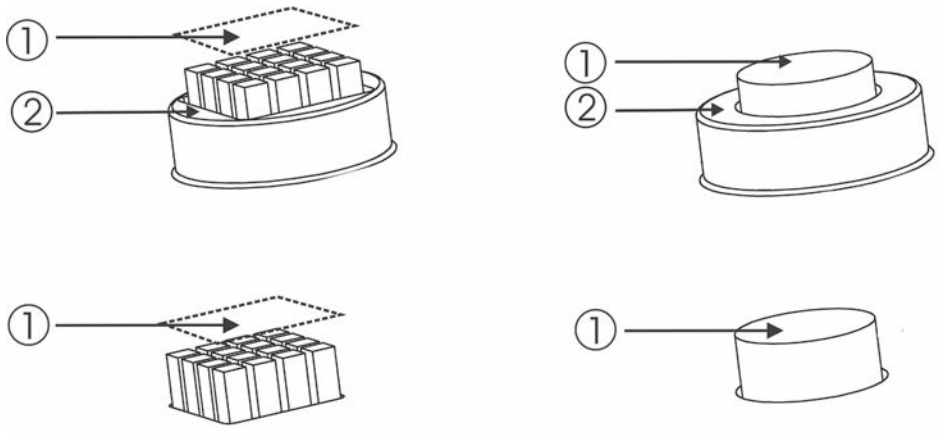

a) Array transducer **b) Single transducer**


Key
1 effective plane
2 auxiliary plane

Figure 1 — Effective plane, auxiliary plane of transducers

3.7
output quantity
electrical signal quantity produced by a transducer, which is a function of a measurand

Note 1 to entry: See Figure 2.

© ISO 2017 – All rights reserved

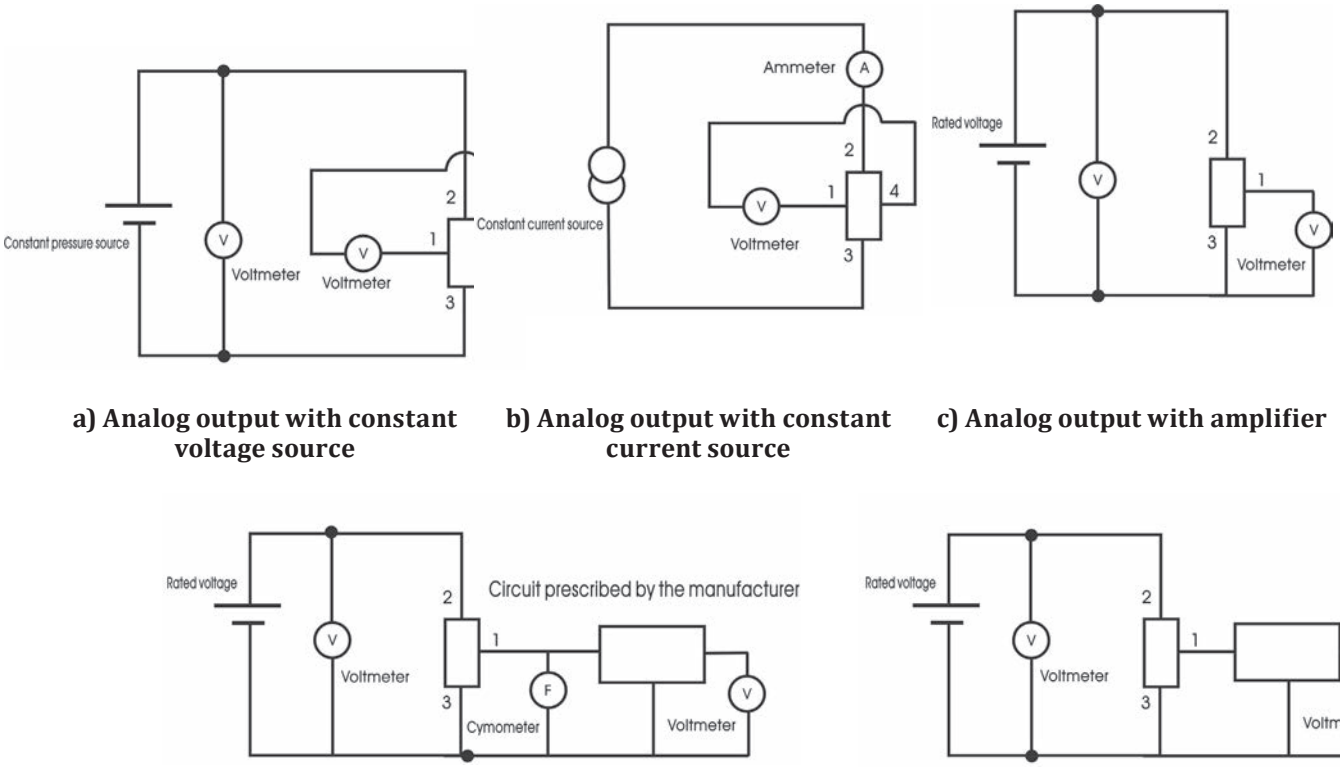

a) Analog output with constant voltage source

b) Analog output with constant current source

c) Analog output with amplifier

d) Frequency output

e) Digital or other forms of output

Key

1 output+
2 input+
3 input-
4 output-

NOTE 1 The output format includes analog output (e.g. a continuous function of a measurand such as changes in voltage amplitude, voltage ratio, and capacitance) which can be classified into amplified and unamplified.

NOTE 2 Frequency output (i.e. the number of cycles or pulses per second as a function of a measurand) and frequency-modulated output (i.e. frequency deviation from a centre frequency) are also forms of analog output.

NOTE 3 Another output format is digital output which represents a measurand in the form of discrete quantities coded in a system of notation (e.g. binary code).

Figure 2 — Different transducers

3.8
resistive bridge transducer
transducer receiving *excitation* (3.11) from alternating or direct electrical energy, the output of which is directly proportional to the product of the applied mechanical quantities and excitation


3.9
static signal
electrical signal transferred from the applied force

Note 1 to entry: See Figure 3.

© ISO 2017 – All rights reserved

3.10
dynamic signal
electrical signal transferred from pulsation at the radial artery and its peripheral tissues detected

Note 1 to entry: See Figure 3.

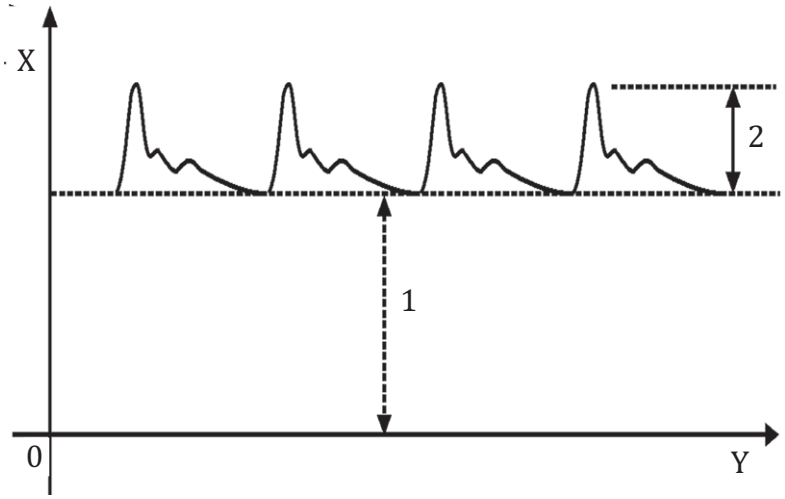

Key
X amplitude
Y time
1 static signal
2 dynamic signal

Figure 3 — Static signal and dynamic signal


3.11
excitation
external energy (voltage or current) applied to a transducer for its proper operation

3.12
measuring range
set of values for a measurand for which the error of the transducer is intended to lie within specified limits

Note 1 to entry: See Figure 4.

[SOURCE: IEC 60747-14-1:2010, 3.2.11]

© ISO 2017 – All rights reserved

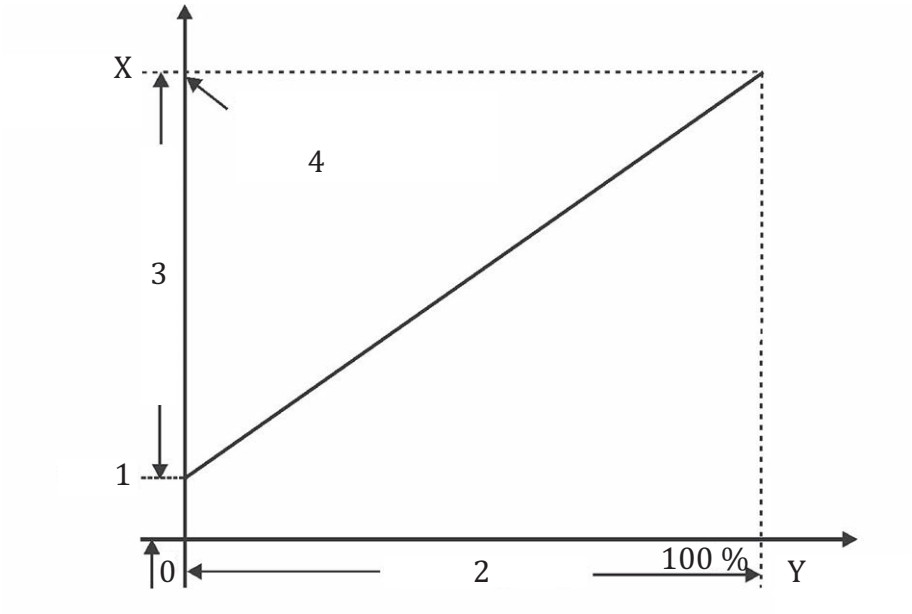

Key

X output (e.g. voltage)
Y measurand (e.g. force)
1 offset
2 measuring range
3 full scale span (FSS)
4 full scale output (FSO); FSO = FSS + offset

Figure 4 — Output-measurand relationship of a linear-output sensor with an offset

3.13
full scale span
FSS
algebraic difference between the end-points of the transducer output

Note 1 to entry: The upper limit of the transducer output over the *measuring range* (3.12) is called the full scale output (FSO). This signal is the sum of the offset signal plus the full scale span.

[SOURCE: IEC 60747-14-1:2010, 3.2.4]

3.14
linearity
closeness between the *calibration* (3.2) curve and a specified straight line of the transducer

Note 1 to entry: This document adopts the end-point or terminal linearity. There are two methods for calculating linearity: end-point straight line fit or a least squares best line fit. While a least squares fit gives the "best case" linearity error, the calculations required are burdensome. Conversely, an end-point fit will give the "worst case" error and the calculations are more straightforward for the user. The result is called the end-point or terminal linearity.

[SOURCE: IEC 60747-14-1:2010, 3.2.7]

3.15
rated load
load value assigned to the transducer by the manufacturer

© ISO 2017 – All rights reserved

3.16
stability
ability of a transducer to maintain its performance characteristics for a certain period of time

Note 1 to entry: Stability is the ability of a transducer to reproduce output readings, obtained during the original calibration, and under constant room conditions, for a specified period of time. It is typically expressed as a percentage of FSO.

[SOURCE: IEC 60747-14-1:2010, 3.2.24]

3.17
hysteresis
maximum difference in output, at any measurand value, within the *measuring range* (3.12) when the value is approached first with an increasing and then a decreasing measurand

Note 1 to entry: Hysteresis is expressed in percent of FSO during one calibration cycle.

[SOURCE: IEC 60747-14-1:2010, 3.2.5]

3.18
drift
undesired change in transducer output, which is irrelevant to the measurand, caused by temperature change at a certain time interval

3.19
repeatability
ability of a transducer to reproduce output readings at room temperature, when the same measurand is applied to it consecutively, under the same conditions and in the same direction


[SOURCE: IEC 60747-14-1:2010, 3.2.17]

3.20
eccentricity
consistency among measurement values of different points applied with identical mechanical quantity on the same *effective plane* (3.4) of the tested transducer under the same measuring conditions

3.21
creep
change in *output quantity* (3.7) within a specified time when applying a measurand to the transducer quickly and then keeping all other external conditions constant

Note 1 to entry: See Figure 5.

© ISO 2017 – All rights reserved

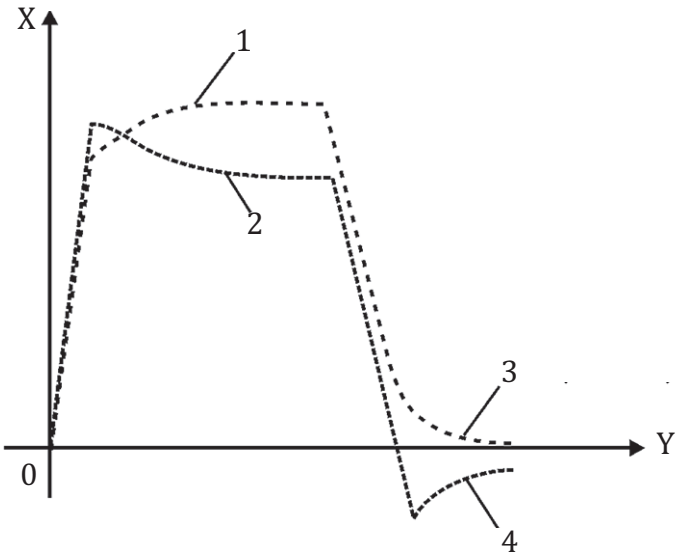

Key

X output
Y time
1 positive creep
2 negative creep
3 positive creep recovery
4 negative creep recovery

Figure 5 — Creep and creep recovery

3.22
input resistance
resistance measured across the *excitation* (3.11) terminal of the transducer

Note 1 to entry: It is sometimes called “excitation resistance”.

3.23
output resistance
effective resistance across the output terminals of the transducer presented to the associated external circuit

Note 1 to entry: It is sometimes called “signal resistance”.

3.24
testing mechanical quantity generator
apparatus which may generate force or pressure to test radial artery mechanical transducer

© ISO 2017 – All rights reserved